

Test Report


nanoe™ X device inhibits activity of adhered methicillin-resistant staphylococcus pseudintermedius (MRSP) by 99.5% in 2 hours

Test outline

- (1) Testing organisation: Nippon Medical School, Nippon Veterinary and Life Science University
- (2) Test subject: Adhered methicillin-resistant staphylococcus pseudintermedius (MRSP)
- (3) Test volume: 45L enclosed box (350×350×400mm)
- (4) Test result: Inhibited 99.5% in 2 hours


Test ambient

45L box

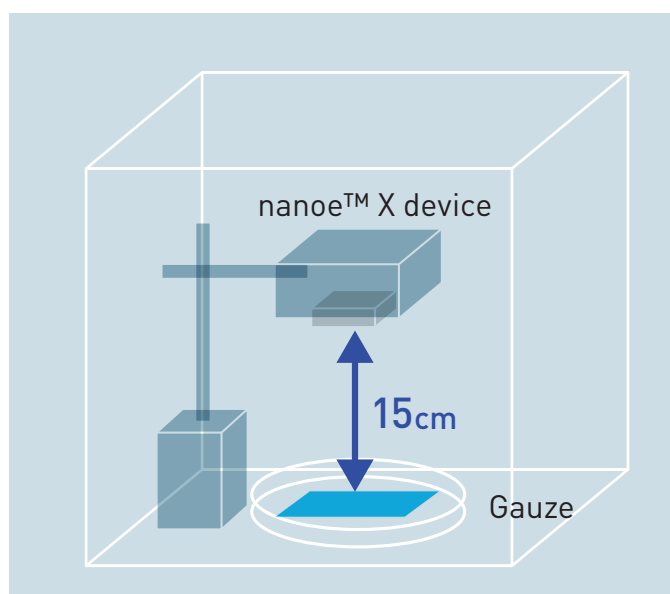

Test result

MRSP

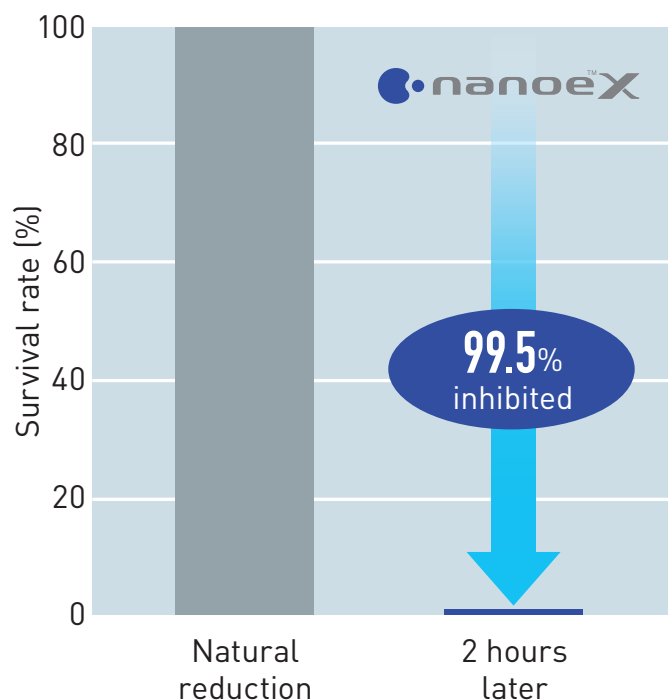

平成 24 年 1 月 27 日

パナソニック株式会社 殿

静電霧化微粒子水(ナノイー)による犬由来病原細菌
(*Staphylococcus pseudintermedius*、*Bordetella*
bronchiseptica、*Pasteurella multocida*) の
不活化効果検証実験

報告書

日本獣医生命科学大学

片岡

