

## Test Report


**nanoe™ X device inhibits activity of adhered  
pasteurella multocida by 99.9% in 1 hour**

### Test outline

- (1) Testing organisation: Nippon Medical School, Nippon Veterinary and Life Science University
- (2) Test subject: Adhered pasteurella multocida
- (3) Test volume: 45L enclosed box (350×350×400mm)
- (4) Test result: Inhibited 99.9% in 1 hour


### Test ambient

45L box

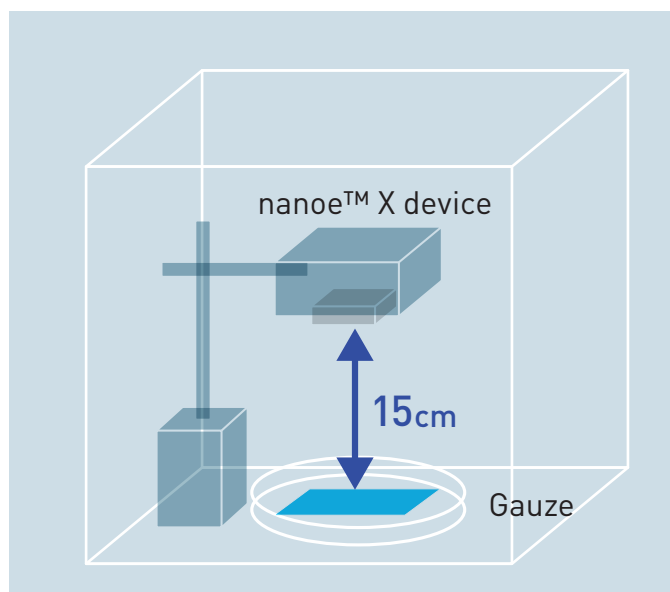

### Test result

Pasteurella multocida

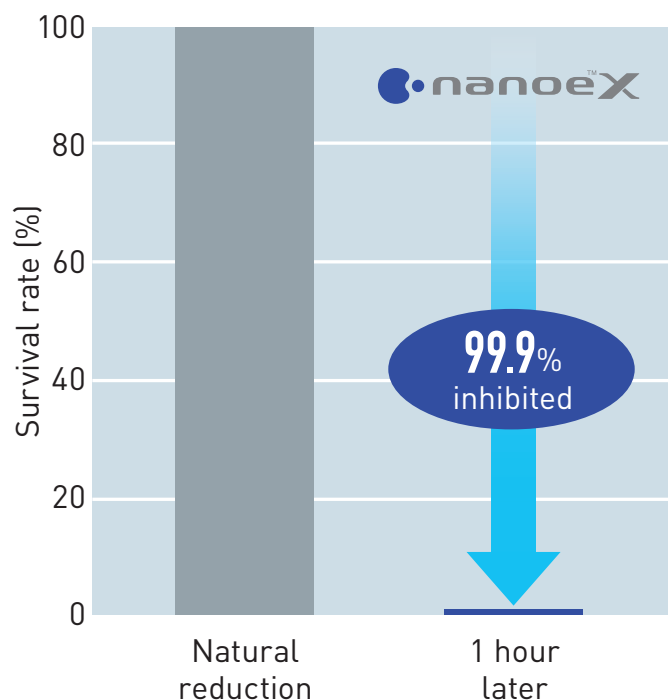

平成 24 年 1 月 27 日

パナソニック株式会社 殿

静電霧化微粒子水(ナノイー)による犬由来病原細菌  
(*Staphylococcus pseudintermedius*、*Bordetella*  
*bronchiseptica*、*Pasteurella multocida*) の  
不活化効果検証実験

報告書

日本獣医生命科学大学

片岡

