

Test Report


An air conditioner equipped with nanoe™ X inhibits activity of adhered rhodotorula mucilaginosa in 8 hours

Test outline

- (1) Testing organisation: Japan Food Research Laboratories
- (2) Test subject: Adhered rhodotorula mucilaginosa
- (3) Test volume: Approx. 24 m³ laboratory (2.73×3.64×2.4m)
- (4) Test result: Inhibited in 8 hours
- (5) Report No.: 18069887001-0201


Test ambient

Approx. 24 m³

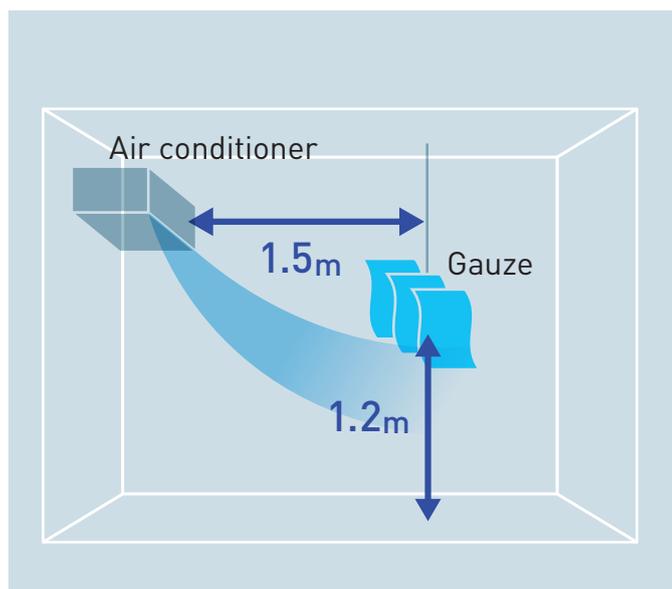

Test result

Rhodotorula mucilaginosa

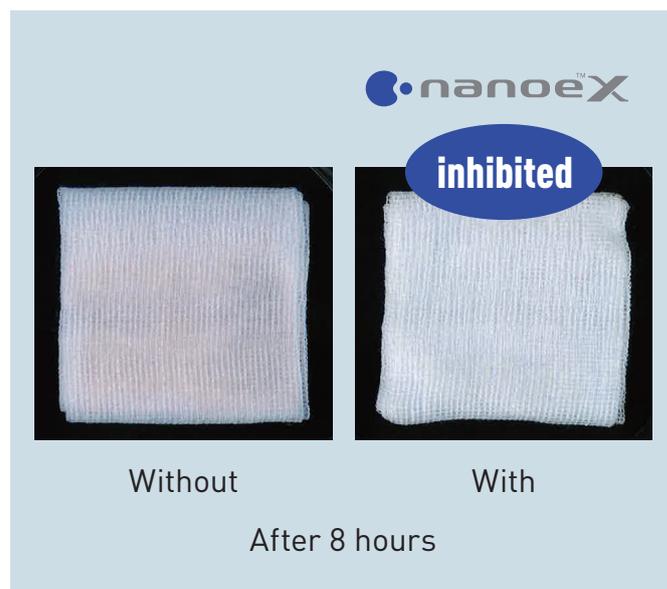

No. 18069887001-0201

Page 1 of 4

Date issued: July 18, 2018

REPORT

Client: Panasonic Corporation
1048 kadoma, kadoma City, Osaka, 571-8686, Japan

Sample(s): nanoeX device

Title: Yeast Growth Test

Received date of sample(s): June 28, 2018

This report has been translated into English from Japanese report No. 18069887001-0101 (Date issued: July 18, 2018).

Signed for and on behalf of JFRL



T. Arai

Takeko Arai
Section of Analysis Documentation

Aug. 07, 2018

Date