

Test Report


**nanoe™ device inhibits activity of adhered
bird flu virus (H5N1 and H9N2 subtypes) by
99.9% in 4 hours**

Test outline


- (1) Testing organisation: Obihiro University of Agriculture and Veterinary Medicine, Research Center for Animal Hygiene and Food Safety
- (2) Test subject: Adhered bird flu virus (H5N1 and H9N2 subtypes)
- (3) Test volume: 45L enclosed box (350×350×400mm)
- (4) Test result: Inhibited 99.9% in 4 hours

Test ambient

45L box

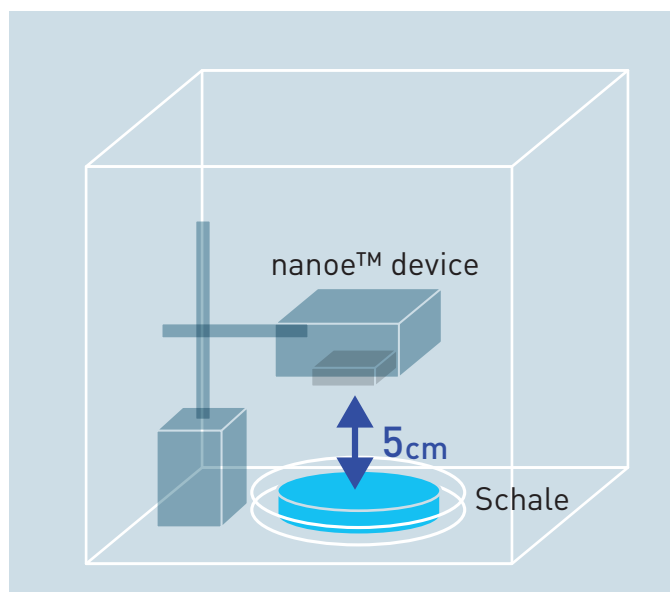

Test result

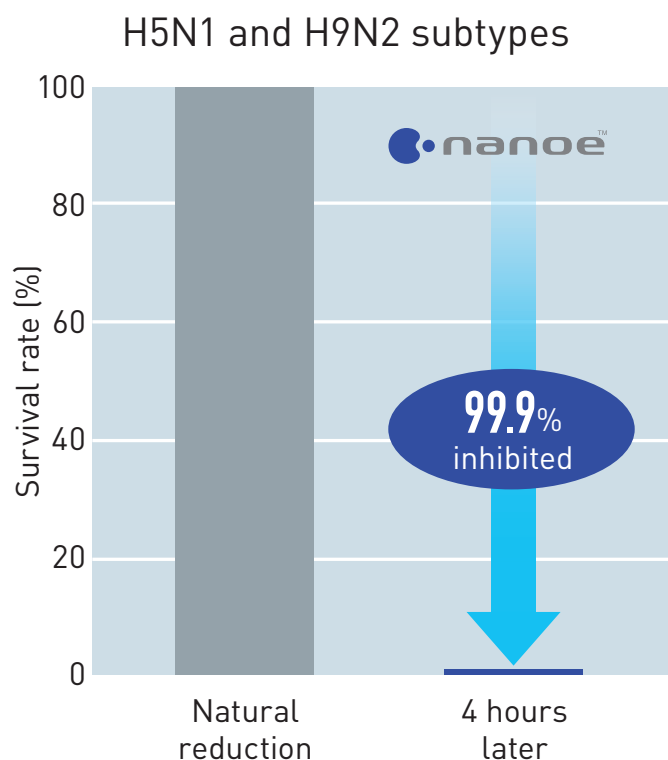

パナソニック電工株式会社 殿

試験報告書

帯電微粒子水のインフルエンザウイルスの形態に及ぼす影響

平成22年3月30日

大動物特殊疾病研究センター・特定疾病分野

今井 小川